



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Eagle Ledge Farm/Mark Dayrell  
625 Maple St  
Grand Ledge MI 48837 U.S.A.

08/14/08

Test No: 334518


### Animal and Sample Description

**Animal Name:** Cisco Kid  
**Breed:** Alpaca(Suri)  
**Sex:** Male  
**Color:** Med Fawn

**Animal ID:** 808887  
**Sample Location:** Side  
**Sample Date:** 05/13/07  
**Age:** 02/14/99

### Laboratory Data

**Mean Fiber Diameter:** 28.2 microns  
**Standard Deviation:** 5.2 microns  
**Coefficient of Variation:** 18.4 %  
**Fibers Greater Than 30 microns:** 29.8 %

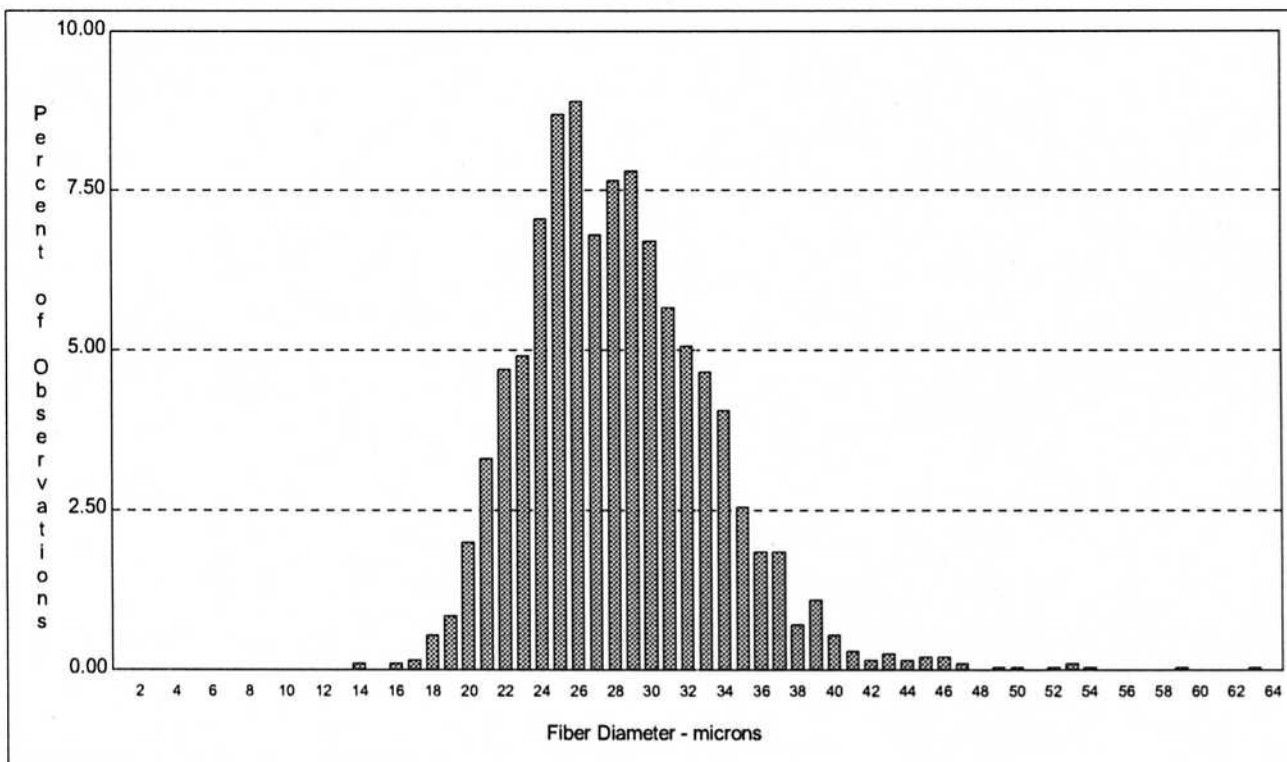

This Test Performed According to I.W.T.O Method 12